

Spiegelberg:

Technology for brains

Silverline[®] 8F subdural drainage catheter **EVD30.015.02**

















Silverline[®] 10F subdural drainage catheter **EVD30.035.02**

Instructions for use

Content

Symbols used	3
General information	3
Technical data	4
Contents of the original packaging.....	4
Approved accessories	4
User group and environment	4
Indications and intended use	5
Contraindications	5
Warnings	5
MRI safety information	6
Application & handling	7
Preparation of the subdural catheter.....	7
Preparation of the application area	7
Insertion of the subdural catheter	8
Tunnelling of the subdural catheter.....	8
Securing the subdural catheter	8
Attaching the connector	9
Connection to an EVD set	9
Checking the function of the subdural catheter.....	9
Drainage of CSF	9
Disconnecting the EVD set	9
Replacing the EVD set.....	9
Closing the wound	10
Determining the position of the subdural catheter	10
Removal of the subdural catheter	10
Disposal.....	10
Returns policy	11

Symbols used

	Item number		Do not use if packaging is damaged.
	Batch number		Upper temperature limit
	Sterilised with ethylene oxide		Caution!
	Do not reuse		Observe instructions for use
	Store in a dry place		Use by
	Keep away from sunlight		Date of manufacture
	Product complies with the requirements of European Directive 93/42/EEC		Manufacturer
	Information note		MR conditional

General information

The instructions for use must be read carefully before use. The product may only be used in accordance with the intended purpose. The manufacturer accepts no liability or warranty for damages caused by improper use or failure to observe the instructions for use.

The product may only be used if the sterile packaging is intact prior to first opening. The product must be transported and stored in a dry place. The following temperatures must be maintained in order to avoid influencing the product properties:

- Transport temperature: up to +50 °C
- Storage temperature: Room temperature
- Ambient temperature for application: Room temperature up to +50 °C

The product is intended for single use only and may not be reused. Reprocessing can lead to the destruction of the product or changes in the product properties. Safe use is therefore no longer guaranteed.

The product must not be cleaned. Only the hose may be moistened with isotonic NaCl solution.

The numbers in brackets refer to the illustration of the product in these instructions for use. In the following, both products are referred to as 'subdural catheters'. If there are additions or exclusions for a product, this is denoted by indicating the reference number. The term "distal" means far from the patient and the term "proximal" means close to the patient.

Technical data

The stated values reflect nominal values and may differ.

REF / Order number	EVD30.015.02	EVD30.035.02
Outer diameter	2.7 mm (8 F)	3.3 mm (10 F)
Drainage lumen inner diameter	1.5 mm	1.9 mm
Drainage hose total length	270 mm	270 mm
Drainage opening diameter	1.2 mm	1.7 mm
Number of openings	48	48
Depth markings	70 – 100 mm (in 5 mm intervals) 150 mm 200 mm	70 – 100 mm (in 5 mm intervals) 150 mm 200 mm
Application duration	Short term up to 30 days	Short term up to 30 days
Material	Silver-impregnated radiopaque polyurethane	Silver-impregnated radiopaque polyurethane

Contents of the original packaging

- 1 subdural catheter
- 1 mandrel
- 1 trocar
- 1 Luer lock connector
- 1 slotted suture attachment
- 1 end cap
- 1 instruction manual

Double packed
EO sterilised
For single use only

Approved accessories

- EVD30.001.01/FV800P External ventricular drainage set (EVD set)
- EVD30.004.01 External ventricular drainage set (EVD set) with plate and clamp
- EVD30.106.01 External ventricular drainage bag

User group and environment

The subdural catheter may only be positioned by a neurosurgeon. Further handling can be done by persons, who have completed medical training and have experience in dealing with neurological trauma (intensive care nurses).

The products are intended exclusively for use in professional healthcare facilities.

Indications and intended use

The subdural catheter drains cerebrospinal fluid (CSF) in adults for the treatment of chronic subdural haematomas. The proximal end is inserted into the subdural cavity for this purpose. The distal end is connected to a droplet chamber system (EVD set) or a drainage bag.

The subdural catheter is impregnated with a silver additive to reduce the probability of microbial colonisation of its surface.

CSF drainage is indicated for the following conditions, for example: traumatic brain injuries, acute hydrocephalus, subarachnoid haemorrhage (SAH), tumours and inflammatory conditions of the medulla oblongata.

Contraindications

The subdural catheter must not be used for purposes other than those specified. Components that have come into contact with infected tissue should not be used further.

Use is always contraindicated in cases of scalp infections, patients receiving anticoagulant therapy and increased bleeding tendency. It is also contraindicated when continuous monitoring by trained personnel cannot be guaranteed.

Warnings



Possible complications when using the subdural catheter include dislocations, bleeding and infections.



Care and caution should be exercised when handling the subdural catheter.



Do not pull on or jerk the subdural catheter quickly! Quickly pulling on or jerking the probe can damage the hose.



Avoid kinks in the hose, as this will impair the drainage.



The subdural catheter must be checked for completeness prior to use. If the product is not complete, the subdural catheter must not be used.



The Luer lock connector (7) must not be disinfected or moistened, as the material may become brittle. This may result in a loss of function of the subdural catheter.



The depth of the subdural catheter can be checked using the marked scale (2).



The subdural catheter must be protected from sunlight and kept away from sources of radiation. Radiation can lead to a deterioration in material properties and thus to the failure of the device functionality.



An open or damaged system must not be used further and must be replaced! Otherwise there is a risk of infection or loss of function.



It is essential that the supplied components are used in order to guarantee compatibility with the subdural catheter.



The mandrel (3) must not be inserted into a subdural catheter which has already been positioned. This poses a risk of injury!



No liquids or drugs may be administered via the subdural catheter.



Check the connections for leaks on a regular basis. Should there be a leaking connection, this poses a risk of contamination or overdrainage.



The procedure for using the subdural catheter must be observed and followed in the correct order.




The position of the subdural haematoma should be checked using imaging techniques prior to application.



Contaminated components and subdural catheters must not be reused.



If problems occur during tunnelling or components become detached, a new subdural catheter should be used.

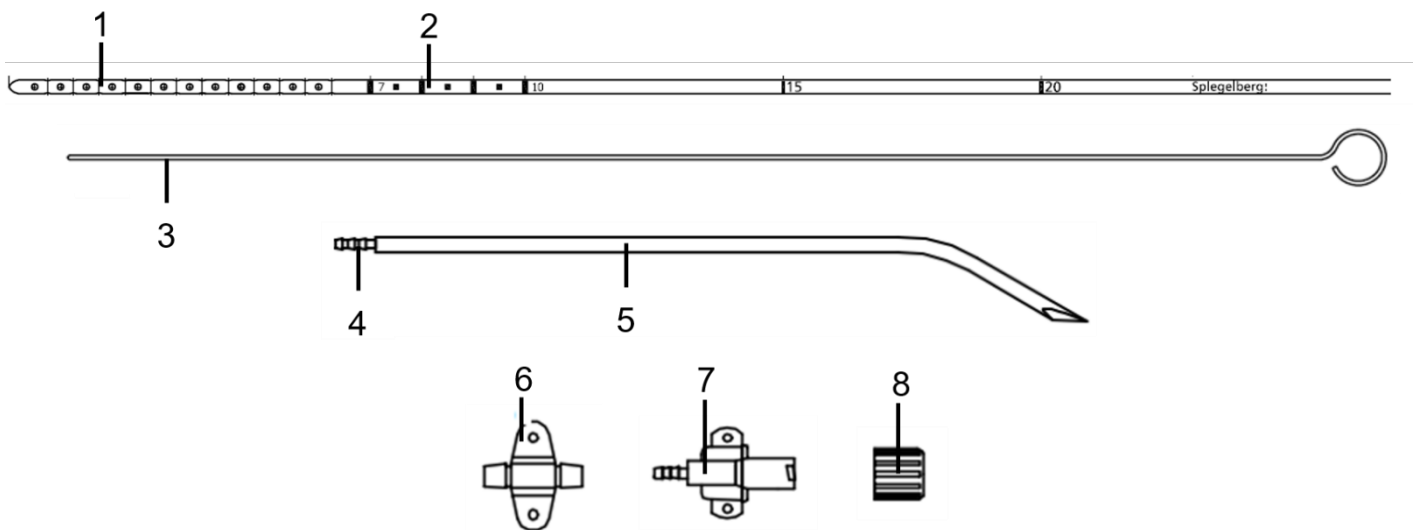

EVD30.015.01 / EVD30.035.01



MR safety information

Non-clinical testing has shown that the “Intracranial Pressure and Catheter System” is “MR conditional”. A patient with this product can be safely scanned in an MRI system meeting the following conditions:

- static magnetic field of 1.5 - 3 tesla with
- maximum spatial field gradient of 2,300 G/cm (23 T/m)
- maximum force product of 38,000,000 G²/cm (38 T²/m)
- theoretically estimated whole body averaged (WBA) specific absorption rate (SAR) < 2 W/kg (Normal Operating Mode).

Under the scanning conditions defined above, the “Intracranial Pressure and Catheter System” is expected to produce a maximum temperature rise of less than

- 2.8 °C (2 W/kg, 1.5 tesla) with an ambient temperature increase of approximately 1.1 °C (2 W/kg, 1.5 tesla)¹
- 2.7 °C (2 W/kg, 3 tesla) with an ambient temperature increase of approximately 0.8 °C (2 W/kg, 3 tesla)²

after 15 minutes of continuous scanning.

In non-clinical tests, the image error generated by the product is around 70.9 mm for the product family worst case³ when the image is generated using a gradient echo pulse sequence and a 3 tesla MRI.



WARNINGS according to the MRI safety information

- Patient injuries can occur if the conditions for safe use in rooms designated as MRI environments are not observed.
- Never exceed a maximum whole body averaged (WBA) specific absorption rate (SAR) of 2 W/kg during MRI measurement (Normal Operating Mode).
- Make sure that all components of the EVD set used with the subdural catheter are “MR safe” or “MR conditional” at 1.5 or 3 tesla.
- Do not bring catheter accessories (mandrel, 3, and trocar, 5) into the MRI environment.

Application & handling

Preparation of the subdural catheter

The subdural catheter should be checked for completeness prior to use.

The insertion depth of the subdural catheter should be determined using imaging techniques prior to insertion.



WARNING! There is a risk of tissue damage if the subdural catheter is inserted too far.



NOTE! If the printed image on the scale (2) is not clearly legible, another subdural catheter must be used.

Preparation of the application area



NOTE! The appropriate insertion site and technique must be selected by the surgeon.

1. Perform aseptic preparation of the surgical area and put up surgical drapes.
2. Open up the scalp.
3. Place a drill hole which is as large as possible (minimum diameter: 3.5 mm for EVD30.015.02 or 4.0 mm for EVD30.035.02).
4. Clean the drill hole completely to remove any chips, splinters and bone fragments.
5. Incise the dura.
6. Place the end cap (8) on the plastic end of the Luer lock connector (7).

¹ RF-related temperature increase for probe 3PS (REF: SND13.1.63/FV535P); worst case on behalf of the whole “Intracranial Pressure and Catheter System” under the aforementioned scanning conditions

² RF-related temperature increase for Silverline® ventricular drainage catheter with cranial screw (REF: EVD30.014.02); worst case on behalf of the whole “Intracranial Pressure and Catheter System” under the aforementioned scanning conditions

³ Determined using the Silverline® ventricular drainage catheter with cranial screw (REF: EVD30.014.02); worst case on behalf of the whole “Intracranial Pressure and Catheter System”.



WARNING! Care should be taken during drilling to avoid drilling too deep and damaging the dura.



WARNING! The mandrel (3) may not be used to open the dura. This may cause damage to the tissue or to the mandrel (3).



NOTE! If the drill hole is too small, it will not be possible to insert the subdural catheter or insertion will not be possible without causing damage.



NOTE! If the drill hole is not cleaned completely to remove any chips, splinters and bone fragments, the subdural catheter may be damaged during insertion.

Insertion of the subdural catheter



NOTE! The mandrel (3) may not be used to insert the subdural catheter. This is associated with a risk of tissue injury or damage.

1. Remove the mandrel (3) from the subdural catheter.
2. Position the subdural catheter in the subdural cavity.
3. Determine the correct depth using the printed scale (2).
4. Check the correct positioning based on the flow of cerebrospinal fluid or blood.

Tunnelling of the subdural catheter



WARNING! The trocar (5) has a sharp tip. There is a risk of injury if the trocar (5) is not handled carefully.

1. Remove the protective cap on the trocar (5).
2. Insert the pointed end of the trocar (5) into the incision above the drill hole.
3. Carefully tunnel the trocar (5) at an appropriate distance from the drill hole. The rear end of the trocar (4) should remain free.
4. Fully push the distal end of the subdural catheter onto the proximal end of the trocar (4).
5. Move the trocar (5) completely under the scalp. There should be no further loops above the drill hole.
6. Clamp the subdural catheter with atraumatic forceps.
7. Cut off the subdural catheter near to the end of the trocar (4).



WARNING! The trocar must be tunnelled away from the drill hole.



NOTE! Do not use force to pull on the hose.



WARNING! If the tunnel is too large, the probability of infection increases due to the larger incision.


Securing the subdural catheter

1. Position the slotted suture attachment (6) on the subdural catheter.
2. Affix the slotted suture attachment (6) to the patient's scalp.



NOTE! The slotted suture attachment (6) should not be affixed in a straight line to the drill hole. Rather, it should be secured in such a way that the hose forms a semicircle shape.

 **NOTE!** The resulting loop should be covered with a bandage to prevent it from becoming caught on the hose and the ICP probe being pulled out.


 **WARNING!** The suture used to attach the slotted suture attachment (6) must not be overtightened. Otherwise the hose may be constricted, resulting in decreased drainage function.

Attaching the connector

Push the distal end of the subdural catheter over the entire length of the metal part of the Luer lock connector (7).


Connection to an EVD set

1. Remove the end cap (8) from the Luer lock connector (7).
2. Connect the Luer lock connector (7) to the connector on the EVD set.
3. Turn the Luer lock connector (7) until significant resistance can be felt and the connection is secure.
4. Perform a visual check for leaks and function.

 **NOTE!** Visual checks of the connection to the EVD set must be carried out on a regular basis.


Checking the function of the subdural catheter

Check the function of the subdural catheter using the CSF flow.

 **NOTE!** Where there is no flow of CSF, this indicates a blockage, kink or constriction. In the event of a blockage, the subdural catheter must be replaced.

Drainage of CSF

Sanguineous CSF in the subdural cavity passes through the drainage holes (1) into the EVD set. If there is no flow of CSF, the hose system must be checked for kinks or constriction.

 **NOTE!** Kinks and constriction in the subdural catheter must be avoided to prevent drainage restrictions.

Disconnecting the EVD set

1. Turn the Luer lock connector (7) counter clockwise.
2. Quickly cap the Luer lock connector (7) with the end cap (8).

Replacing the EVD set

1. Disconnect the Luer lock connector (7) and the EVD set.
2. Quickly cap the Luer lock connector (7) with the end cap (8).
3. Replace the EVD set according to the manufacturer's instructions.
4. Remove the end cap (8) from the Luer lock connector (7).
5. Connect the Luer lock connector (7) to the EVD set.

Closing the wound

After the proper function of the subdural catheter has been confirmed, the wound on the scalp can be closed. The technique and material used for this are to be determined by the surgeon.

i **NOTE!** When closing the wound, care must be taken not to damage the subdural catheter.

i **NOTE!** Ensure that the subdural catheter is not constricted while closing the wound. Otherwise the drainage may become blocked.

Determining the position of the subdural catheter

The position of the subdural catheter can be checked using imaging techniques.

i **NOTE!** The correct positioning of the subdural catheter and the condition of the patient must be checked at regular intervals.

Removal of the subdural catheter

i **NOTE!** Proceed slowly and carefully when removing the subdural catheter. It must be ensured that no tissue is damaged and that the slotted suture attachment (6) has been detached.

i **NOTE!** The subdural catheter must not be removed in a fast and jerky manner in order to avoid injuries and prevent blood, CSF and possibly tissue from being sprayed around.

i **NOTE!** The subdural catheter must not be pulled over sharp or uneven edges during removal to avoid damaging the hose and possibly tearing the subdural catheter.

1. Disconnecting the subdural catheter and the EVD set.
2. Loosen the fixings attaching the subdural catheter to the patient.
3. Pull out the subdural catheter.
4. Check that the subdural catheter has been removed completely and that the tissue has not been damaged.
5. Observe the condition of the patient.

i **NOTE!** No components of the subdural catheter may be left in the patient.

Disposal

After use, the product should be disposed of in accordance with the regulations for infectious waste and/or in accordance with national or regional regulations.

Returns policy

Before returning a product, approval must be obtained from the customer service department. Returns will not be accepted unless the return has been approved in advance by Spiegelberg in the context of a complaint or a return has specifically been requested.

Contaminated/used products must be packaged in a bag for biological hazardous substances for return shipment.



Manufacturer:
Spiegelberg GmbH & Co. KG
Tempowerkring 4
21079 Hamburg
Germany

Tel.: +49-40-790-178-0
Fax: +49-40-790-178-10
E-mail: info@spiegelberg.de
<http://www.spiegelberg.de>

Subject to technical changes.
Version: 12 / 2020-11-09



0297

© by Spiegelberg GmbH & Co. KG 2020